

Hybrivet Systems, Inc.

17 Erie Drive Natick, MA 01760 (508)651-7881 Fax: (508)651-8837 www.LeadCheck.com

August 30, 2006


LeadCheck[®] Aqua II

The standard protocol for the detection of lead in water was followed at the level of 15 ppb. The developed strips are illustrated below.

These strips were developed as usual.



These strips were developed as usual and then washed lightly with water to remove background.

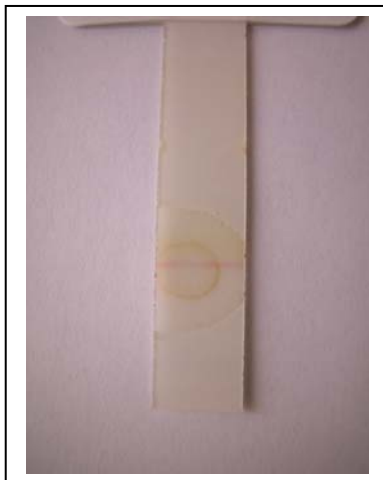

The above results are expected for 15 ppb lead in water.